# Shamrock labels

## Tapes & Labels

FOR MEDICAL IMAGING & RESPIRATORY CARE





## Shamrock's Mission

Our mission is to supply quality, innovative labeling systems to the healthcare industry that help protect patient safety, fulfill modern technological needs and remain cost effective.



## **Environmental Policy**

It is Shamrock's policy to provide a safe and healthy workplace for our employees and to be an environmentally responsible neighbor in our community. From product manufacture through shipping, in both office and production facilities, Shamrock supports comprehensive programs designed to positively impact the safety of our population and natural resources.



# Joint Commission National Patient Safety Goals

For Medical Imaging & Respiratory Care

#### Sustained with Shamrock Labels

**Goal 1**. Improve the accuracy of patient identification.

**Goal 2.** Improve the effectiveness of communication among caregivers.





## Medical Imaging & Respiratory Care

BLANK LABELS FOR	Thermal Printer Labels	MI-2
ON-DEMAND PRINTING	Laser Printer Labels	MI-3
	Dot Matrix Printer Labels	MI-3
COLOR CODED FILING LABELS	Style A Labels	MI-4
	Style S Labels	MI-4
	Style T Labels	MI-5
	File Folder Correction Labels	MI-5
COMMUNICATION LABELS	Informational Labels	MI-6
	Mailing Labels	MI-6
	Position Labels	MI-6
	Pre-Printed Disc Labels	MI-6
	Alert Labels	MI-7
	X-Ray Labels	MI-7
	MRI Labels	MI-7
	C.T. Labels	MI-7
METRIC MEASURE LABELS	Metric Measure Labels	MI-7
DATE LABELS	Standard & Color Coded Date Labels	MI-8
	2	141.5
LABELS FOR DIAGNOSTIC IMAGING	Contrast Labels	MI-8
	Radiopharmaceutical Labels	MI-8
LADELS FOR MUCLEAR MEDICINE	Dadisastisa Wassing Labela 0 Tanas	MLO
LABELS FOR NUCLEAR MEDICINE	Radioactive Warning Labels & Tapes	MI-9
	Communication Labels	MI-9
	Shipping Labels	MI-9
LABELS FOR RESPIRATORY CARE	Objective and Evaluation Labels	MI-10
LABELS FOR RESPIRATORT CARE	Communication Labels	MI-10
	Equipment Labels	MI-11
PRODUCTS FOR COLOR CODING	Labeling Tape	MI-12
	Dot Labels	MI-12
	Tape Dispensers	MI-12

## Specialty Blank Labels for On-Demand Printing

## **Specialty Labels for Thermal Printers**

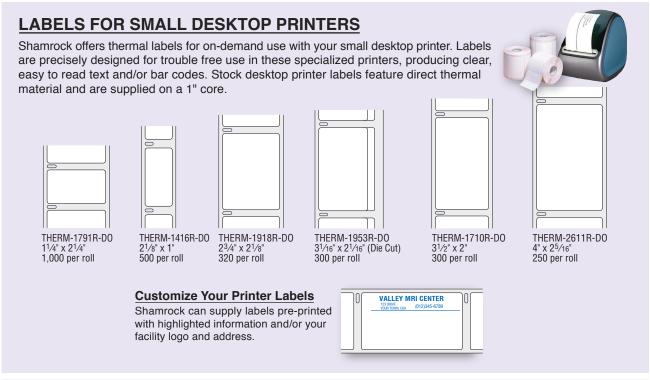


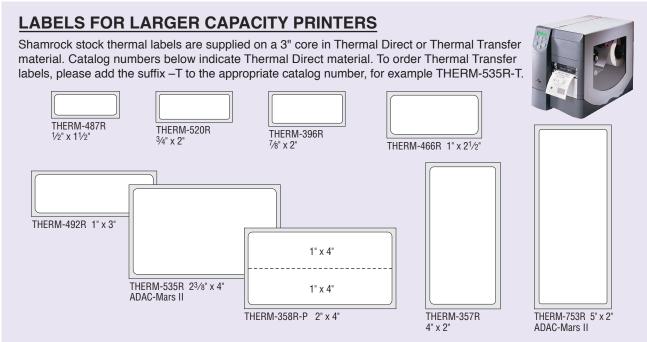


SHAMROCK LABELS 34 DAVIS DRIVE, BELLWOOD, ILLINOIS 60104



## Specialty Labels for Laser Printers

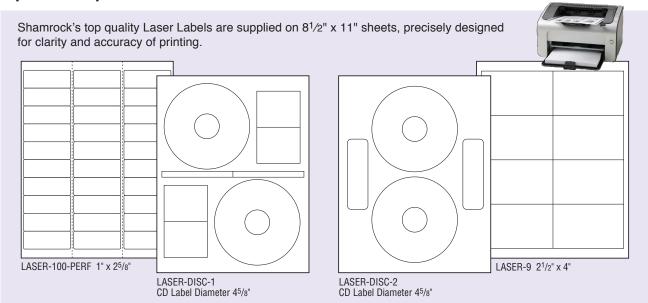

## Specialty Labels for Dot Matrix Printers

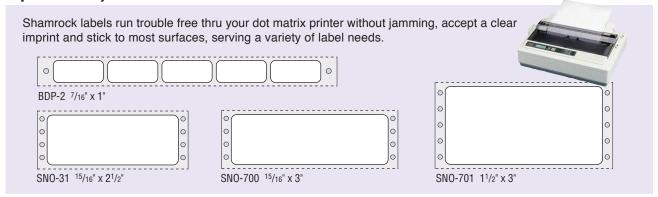

## Color Choices for all Specialty Blank Labels



## Specialty File Folder Labels

#### **COLOR CODED FILING LABELS**

Shamrock's color coded Filing Labels feature brilliant colors and strong, permanent adhesive. Labels in each style are laminated to stand up to frequent use and scored to fold easily. When ordering, select the prefix FX (color only), FXN (color and number), FXY (color and year), FXA (color and letter) or FXM (color and month) and the appropriate number suffix as listed for the label style you have chosen. For instance a Style T label, showing the number 6, would be ordered as FXN-506.


17/8" x 17/8" LABELS



#### STYLE A LABELS offer options in label and imprint sizes. 1,000 labels per roll.









1/2" x 13/4" LABELS **Color Only** FX-3000 Series

FX-3006 Yellow Color & Small Numbers FXN-3000 Series

9 FXN-3009 Green

## **COLOR NUMBERS**

Style A Labels
300 & 3000 - Red
301 & 3001 - Gray
302 & 3002 - Blue
303 & 3003 - Orange
304 & 3004 - Purple
305 & 3005 - Black
306 & 3006 - Yellow
307 & 3007 – Brown
308 & 3008 - Pink
309 & 3009 - Green

#### STYLE A LABELS month. 1,000 labels per roll.

1/2" x 13/4" LABELS Color & Month FXM-300 Series **DEC** DEC FXM-321 Red

Style	A Color	& Month
JAN	FXM-310	Gray
FEB	FXM-311	Dark Blue
MAR	FXM-312	Dark Green
APR	FXM-313	Purple

#### Style A Color & Month MAY FXM-314 White JUN FXM-315 Yellow FXM-316 JUL Brown FXM-317 AUG Pink

Style	Α	Color	& Month
SEP	F)	KM-318	Black
OCT	F)	KM-319	Orange
NOV	F)	KM-320	Blue
DEC	F)	XM-321	Red

#### STYLE S LABELS provide a different color coding scheme. 1,000 labels per roll.







COLOR NUMBERS Style S Labels
400 - Yellow
401 – Blue
402 – Pink
403 – Purple
404 – Orange
405 – Brown
406 – Green
407 – Gray
408 – Red
409 – Black

#### STYLE S LABELS month. 1,000 labels per roll.



Style	S Color	& Month
JAN	FXM-410	Dark Green
FEB	FXM-411	Purple
MAR	FXM-412	Blue
APR	FXM-413	Brown

Style	S Color	& Month
MAY	FXM-414	Black
JUN	FXM-415	Gray
JUL	FXM-416	Red
AUG	FXM-417	Yellow

Style	S	Color	& Month
SEP	FX	M-418	Pink
OCT	FX	M-419	Orange
NOV	FX	M-420	Lavender
DEC	FX	M-421	Light Green





#### STYLE T LABELS offer a third color coding scheme. 1,000 labels per roll.







#### 7/8" x 17/8" LABELS

Color & Year FXY-500 Series FXY-508 Lavender

### **COLOR NUMBERS**

Style T Labels
500 – Pink
501 – Red
502 – Light Orange
503 - Dark Orange
504 – Light Green
505 – Dark Green
506 – Blue
507 – Purple
508 – Lavender
509 – Brown

#### STYLE T LABELS month. 1,000 labels per roll.

7/8" x 17/8" LABELS Color & Year



Style	T Color	& Month
JAN	FXM-510	Dark Green
FEB	FXM-511	Dark Blue
MAR	FXM-512	Blue
APR	FXM-513	Brown

#### Style T Color & Month MAY FXM-514 Black FXM-515 Gray JUN JUL FXM-516 Red

FXM-517 Yellow

Style	T Color	& Month
SEP	FXM-518	Pink
OCT	FXM-519	Orange
NOV	FXM-520	Purple
DEC	FXM-521	Green

#### STYLE T ALPHA LABELS offer a distinct color format for every letter. 500 labels per roll.

AUG

1" x 11/2" LABELS



FXA-500	) Serie:	s (solid)
A	ļ	A
FXA-	501-A	Red

Style T Alpha Labels

Red (solid)

Blue (solid)

Purple (solid)

Lavender (solid)

Pink (one bar)

Light Orange (solid)

Dark Orange (solid)

Light Green (solid)

Dark Green (solid)

FXA-501-A

FXA-502-B

FXA-503-C

FXA-505-E

FXA-506-F

FXA-507-G

FXA-500-I

D FXA-504-D

H FXA-508-H

Α

С

G

#### 1" x 11/2" LABELS



FXA-507-P Purple

1" x 11/2" LABELS

Color & Alpha FXA-500 Series (two bars)



St	yle T	Alpha	Labels
----	-------	-------	--------


J	FXA-501-J	Red (one bar)
K	FXA-502-K	Light Orange (one bar)
L	FXA-503-L	Dark Orange (one bar)
M	FXA-504-M	Light Green (one bar)
Mo	FXA-504-Mc	Light Green (one bar)
N	FXA-505-N	Dark Green (one bar)
0	FXA-506-0	Blue (one bar)
P	FXA-507-P	Purple (one bar)
Q	FXA-508-Q	Lavender (one bar)

Style T Alpha Labels

R	FXA-509-R	Brown (one bar)
S	FXA-500-S	Pink (two bars)
Τ	FXA-501-T	Red (two bars)
U	FXA-502-U	Light Orange (two bars)
٧	FXA-503-V	Dark Orange (two bars)
W	FXA-501-W	Dark Green (two bars)
Χ	FXA-501-X	Blue (two bars)
Υ	FXA-501-Y	Purple (two bars)
Z	FXA-501-Z	Lavender (two bars)

#### FILE FOLDER CORRECTION LABELS

These handy, opaque labels fit over incorrect or outdated information, feature a smudge resistant surface and pressure sensitive, permanent adhesive. Supplied 500 labels per roll.



## **Specialty Communication Labels**

#### **INFORMATIONAL LABELS**

Printed on shiny kromekote stock, these labels measure 17/8" x 17/8". Their permanent adhesive holds them securely in place; they won't flag or fall off. Labels are supplied 1,000 per roll.

C.T. SCAN

FXS-100

Mammography

Mammography

**Do Not Destroy** 

FXS-201

MEDICINE NUCLEAR

MEDICINE FXS-101

Do Not Destroy

And to Not Destroy Do Not Destroy

**Do Not Destroy** 

FXS-202

SPECIAL SPECIAL

SPECIAL PROCEDURES

FXS-102

Digital gnigsml

Digital Imaging

FXS-210

ARTJU GNUOS

> ULTRA SOUND


FXS-103



FXS-211

#### **MAILING LABELS**

Have your return address pre-printed on labels featuring smudge resistant surface and permanent adhesive. Supplied 1,000 labels per roll.



SX-101 2<sup>1</sup>/2" x 4"

#### **POSITION LABELS**

Labels are supplied in 1/2" x 500" tape rolls. To order as 1/2" x  $1^{1}/2$ " pre-cut labels on 500" rolls, add the suffix -PRE to the appropriate catalog number below.

Cat. No.	Imprint
SX-30	RIGHT
SX-31	LEFT
SX-33	UPRIGHT
SX-34	RT. LATERAL
SX-38	DECUBITUS
SX-39	PORTABLE
SX-41	AP
SX-50	SUPINE



#### PERSONALIZED COMPACT DISC LABELS


Have labels pre-printed to your specifications. Removable tabs facilitate proper alignment on disc. Permanent adhesive holds label firmly in place during use and storage. Supplied 500 labels per roll.

See page MI-3 for blank Disc Labels for on-site, laser printing.




SX-DISC 5" x 5" Label Diameter 41/4"



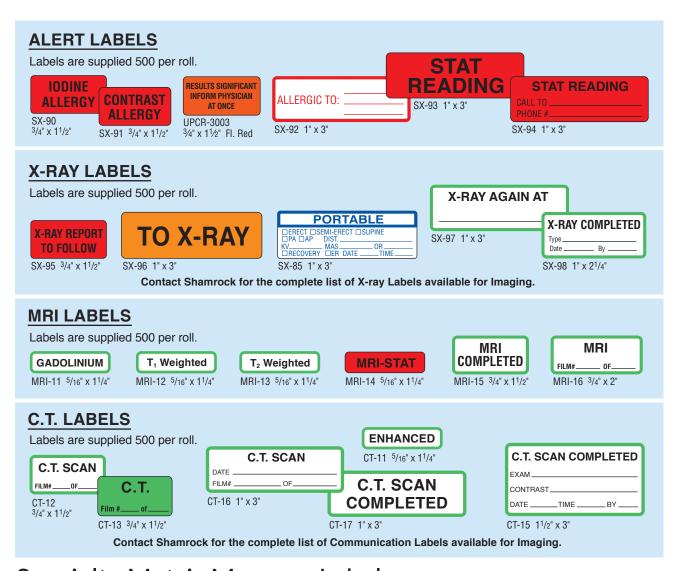

## Specialty Metric Measure Labels

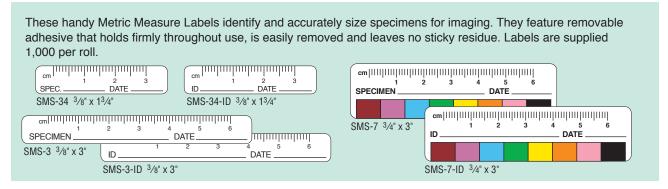

SHAMROCK LABELS  $\,$  34 DAVIS DRIVE, BELLWOOD, ILLINOIS  $\,$  60104

## Specialty Date Labels

#### STANDARD DATE LABELS

Specialty Date Labels identify the correct reading side of the image, provide the date the image was taken and facilitate refiling. Clearly printed in black on yellow litho stock, Specialty Date Labels accept notations in pen, pencil or marker, feature permanent pressure-sensitive adhesive that stays in place, cannot be removed. Labels measure 1/2" x 11/2". Date Labels supplied for each month in a unique dispenser box that includes one roll of labels for each day of the month.





Date-1 (100 labels per roll)


Date-2 (200 labels per roll)


Date-3 (300 labels per roll)

#### **COLOR CODED DATE LABELS**

Printed in a different color for each month, these ½" x 1½" labels tell you immediately the month each film was taken. Large printing and room to inscribe the exact time of exposure increase the information conveyed at a glance. Color Coded Date Labels are priced the same as Shamrock's standard date labels.







Date-10 (100 labels per roll)

Date-20 (200 labels per roll)

Date-30 (300 labels per roll)

## Specialty Labels for Diagnostic Imaging

#### **CONTRAST LABELS**

Shamrock's pre-cut Diagnostic Imaging Syringe Labels provide an economical, easy to use identification system. They may be sterilized by steam or ethylene oxide. Labels are supplied in 500" rolls. Contact Shamrock for a complete list of Diagnostic Imaging Syringe Labels.











SXD-150 3/4" x 13/4"

#### RADIOPHARMACEUTICAL LABELS

Designed for syringe plunger tops, labels measure <sup>1</sup>/<sub>2</sub>" in diameter, feature colors coordinated to most packaging color schemes and are supplied 500 labels per roll. Contact Shamrock for a complete list of Radiopharmaceutical Labels.


















SHAMROCK LABELS 34 DAVIS DRIVE, BELLWOOD, ILLINOIS 60104



## Specialty Labels for Nuclear Medicine

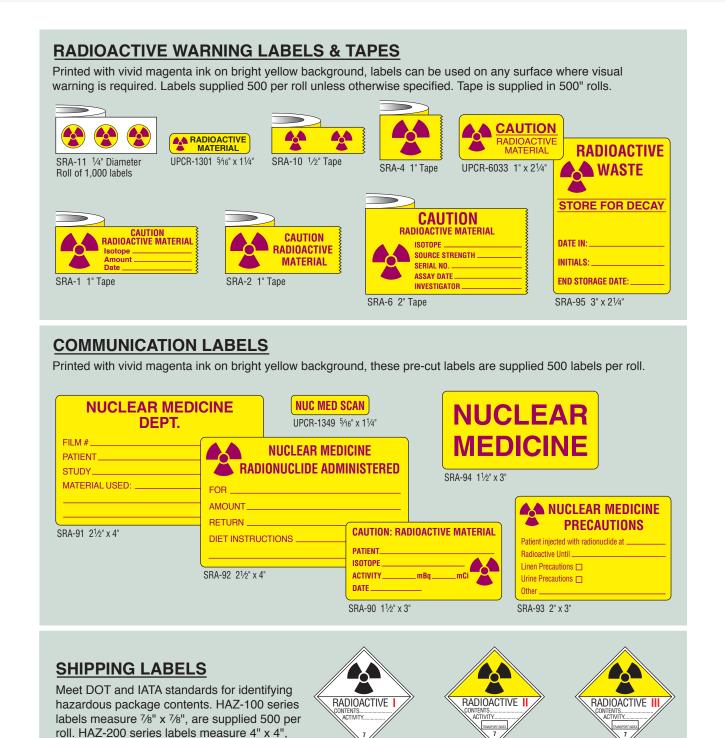

HAZ-116 7/8" x 7/8"

HAZ-117 7/8" x 7/8"

HAZ-217 4" x 4"

are supplied 250 per package.

HAZ-118 7/8" x 7/8"

HAZ-218 4" x 4"

## Specialty Labels for Respiratory Care



Labels for Respiratory Care accept notations in pen, pencil or marker, feature removable adhesive that holds labels firmly in place during use yet is easily removed when appropriate. Contact Shamrock for information on labels designed to your exact specifications. Stock labels are supplied 250 per roll unless otherwise specified.

		RESPIRATOR	Y CARE DEPARTMENT
RESPIRATORY CAR OBJECTIVES OF RESPIRAT			RESPIRATORY REVIEW
		Respiratory Therapy:	
PATIENT NAME	RM#	Type of Therapy	Date Started
Patient has been started on the following F			
		Physician:	y being achieved: ☐ Yes ☐ No
Please indicate the following Objectives for Th	erapy	Comments:	
	deposition of medication		Discontinue
	cal conditioning exercises  ve arterial oxygenation	☐ Change To:	Discontinue
☐ Mobilization of secretions		PLEASE DOCUMENT IN PH	YSICIANS ORDERS
☐ Other: Signature		Date Phys	sician
SRT-50 2 <sup>1</sup> / <sub>2</sub> " x 4" Fl. Chartreuse 1,000	per roll	SRT-54 2 <sup>5</sup> /8" x 4" 1,000 p	er roll
OMMUNICATION LABE	LS		
OVV	CENI C	Respiratory Care Dept.	
OXY	JEIN A	CAUTION	
Pt. Name		MAINTAIN OXYGEN FLOWR	ATE
Date		DateTime	<u> </u>
		By	TRAP 02 TUBING CHANGED
T-61 1" x 4" Perf Down Center For Easy Fold		X 3"	OUND
	Pert at lab t		0 <sub>2</sub> Date Time
RESPIRATORY CARE DEPT.  OXYGEN		TU	BING By
iters/min		Y CARE DEPT.	107.4101
iters/min t. Name	TORING CH	HANGED ON SRT	-67 1" x 3" at Tab to Wrap Around Tubing
		1 011	at tab to wrap mount rabing
RESPIRATORY CARE			
TIEST ITATOTT CALL	ODT 00 7/II 01/II	LEL D. d	DESDIDATORY CARE DEDT
T-62 1" x 21/4" OXYGEN SET AT  — L/Min or % Name	SRT-66 <sup>7</sup> /8" x 2 <sup>1</sup> /4"	' Fl. Red	RESPIRATORY CARE DEPT.
T-62 1" x 21/4" OXYGEN SET AT L/Min or % Name Room	SRT-66 7/8" x 21/4"		RESPIRATORY CARE DEPT.  STERILE
T-62 1" x 21/4" Pink  OXYGEN SET AT  L/Min or % Name  Room  DO NOT ADJUST	SRT-66 7/8" x 21/4"	IRATORY CARE	STERILE
T-62 1" x 21/4" OXYGEN SET AT L/Min or % Name Room	SRT-66 7/8" x 21/4"  RESPI  OXIMETF	RATORY CARE	STERILE NORMAL SALINE
F-62 1" x 2 <sup>1</sup> /4" OXYGEN SET AT L/Min or % Name Room DO NOT ADJUST	SRT-66 7/8" x 21/4"  RESPI  OXIMETF	RATORY CARE	STERILE
OXYGEN SET AT OXYGEN SET AT L/Min or % Name Room DO NOT ADJUST  SRT-65 7/8" x 21/4" Fl. Pink	SRT-66 7/6" x 21/4"  RESPI  OXIMETF  DATE  PT. SITTING	RATORY CARE RY TEST RESULT  TIME  " 02	STERILE NORMAL SALINE SRT-68 1" x 2"
F-62 1" x 2 <sup>1</sup> /4" OXYGEN SET AT L/Min or % Name Room DO NOT ADJUST	SRT-66 7/6" x 21/4"  RESPI  OXIMETF  DATE  PT. SITTING  PT. SUPINE	RATORY CARE RY TEST RESULT  TIME  " 02 L/MIN.	STERILE NORMAL SALINE SRT-68 1" x 2"  RESPIRATORY CARE
OXYGEN SET AT  OXYGEN SET AT  L/Min or % Name  Room  DO NOT ADJUST  SRT-65 7/8" x 21/4" FI. Pink	RESPI OXIMETF  DATE PT. SITTING PT. SUPINE SATURATI	RATORY CARE RY TEST RESULT  TIME % 02 L/MIN	STERILE NORMAL SALINE SRT-68 1" x 2"
T-62 1" x 21/4"  Pink  OXYGEN SET AT  L/Min or % Name  Room  DO NOT ADJUST  SRT-65 7%" x 21/4" FI. Pink	RESPI OXIMETF  DATE PT. SITTING PT. SUPINE SATURATI COMMENTS:	RATORY CARE RY TEST RESULT  TIME % 02 L/MIN 10N%	STERILE NORMAL SALINE SRT-68 1" x 2"  RESPIRATORY CARE DOCTOR
T-62 1" x 21/4"  Pink  OXYGEN SET AT  L/Min or % Name  Room  DO NOT ADJUST  SRT-65 7%" x 21/4" FI. Pink	RESPI OXIMETF  DATE PT. SITTING PT. SUPINE SATURATI COMMENTS:	RATORY CARE RY TEST RESULT  TIME % 02 L/MIN 10N%	STERILE NORMAL SALINE SRT-68 1" x 2"  RESPIRATORY CARE DOCTOR  OXIMETRY DONE:
T-62 1" x 21/4"  Pink  OXYGEN SET AT  L/Min or % Name  Room  DO NOT ADJUST  SRT-65 7%" x 21/4" FI. Pink	RESPI OXIMETF  DATE PT. SITTING PT. SUPINE SATURATI COMMENTS: THERAPIST	RATORY CARE RY TEST RESULT  TIME % 02 L/MIN ION%	STERILE NORMAL SALINE SRT-68 1" x 2"  RESPIRATORY CARE DOCTOR  OXIMETRY DONE:EAR  DATE:
T-62 1" x 21/4" Pink  OXYGEN SET AT  L/Min or % Name  Room  DO NOT ADJUST  SRT-65 7/8" x 21/4" FI. Pink	RESPI OXIMETF  DATE PT. SITTING PT. SUPINE SATURATI COMMENTS:	RATORY CARE RY TEST RESULT  TIME % 02 L/MIN ION%	STERILE NORMAL SALINE SRT-68 1" x 2"  RESPIRATORY CARE DOCTOR  OXIMETRY DONE: — EAR — PULSE  TIME: — TIME:
T-62 1" x 21/4" Pink  OXYGEN SET AT  L/Min or % Name  Room  DO NOT ADJUST  SRT-65 7/8" x 21/4" FI. Pink	RESPI OXIMETF  DATE PT. SITTING PT. SUPINE SATURATI COMMENTS: THERAPIST  SRT-69 2" x 3" F	RATORY CARE RY TEST RESULT  TIME % 02 L/MIN ION%	STERILE NORMAL SALINE SRT-68 1" x 2"  RESPIRATORY CARE DOCTOR  OXIMETRY DONE:EARPULSE TIME:ROOM AIR SATURATION:%
T-62 1" x 21/4" Pink  OXYGEN SET AT  L/Min or % Name  Room  DO NOT ADJUST  SRT-65 7/8" x 21/4" FI. Pink	RESPI OXIMETF  DATE PT. SITTING PT. SUPINE SATURATI COMMENTS: THERAPIST	RATORY CARE RY TEST RESULT  TIME % 02 L/MIN ION%	STERILE NORMAL SALINE SRT-68 1" x 2"  RESPIRATORY CARE DOCTOR  OXIMETRY DONE:EARPULSE TIME:PULSE TIME:%  0_2@L/MIN. SATURATION:%
T-62 1" x 21/4" Pink  OXYGEN SET AT  L/Min or % Name  Room  DO NOT ADJUST  SRT-65 7/8" x 21/4" FI. Pink	RESPIOXIMETE DATE PT. SITTING PT. SUPINE SATURATI COMMENTS: THERAPIST SRT-69 2" x 3" FI	RATORY CARE RY TEST RESULT  TIME  % 02  L/MIN.  ION  %	STERILE NORMAL SALINE SRT-68 1" x 2"  RESPIRATORY CARE DOCTOR  OXIMETRY DONE:EARPULSE TIME:ROOM AIR SATURATION:%
T-62 1" x 21/4"  Pink  OXYGEN SET AT  L/Min or % Name  Room  DO NOT ADJUST  SRT-65 7%" x 21/4" FI. Pink	RESPI OXIMETF  DATE PT. SITTING PT. SUPINE SATURATI COMMENTS: THERAPIST  SRT-69 2" x 3" F	RATORY CARE RY TEST RESULT  TIME  % 02  L/MIN.  ION  %	STERILE NORMAL SALINE SRT-68 1" x 2"  RESPIRATORY CARE DOCTOR  OXIMETRY DONE: — EAR — PULSE TIME: — PULSE TIME: — ROOM AIR SATURATION: — % COMMENT:
T-62 1" x 21/4"  Pink  OXYGEN SET AT  L/Min or % Name  Room  DO NOT ADJUST  SRT-65 7%" x 21/4" FI. Pink	RESPIOXIMETE DATE PT. SITTING PT. SUPINE SATURATI COMMENTS: THERAPIST SRT-69 2" x 3" FI	TIME	STERILE NORMAL SALINE SRT-68 1" x 2"  RESPIRATORY CARE DOCTOR  OXIMETRY DONE:EARPULSE TIME:PULSE TIME:%  0_2@L/MIN. SATURATION:%

SHAMROCK LABELS 34 DAVIS DRIVE, BELLWOOD, ILLINOIS 60104



RESPIRATORY CARE DEPTY WENTILITOR CHECKLIST WANAY  SRT-44 3/4' x 4" FI. Red Perf Down Center For Easy Fold Over  Respiratory Use Only Respiratory Care Dept. FOUNDMENT CHANGED DATE NITTAL SRT-72 3/4' x 2" FI. Green  RESPIRATORY CARE DEPT. EQUIPMENT CHANGED DATE NITTAL SRT-72 3/4' x 2" FI. Green  RESPIRATORY CARE DEPT. EQUIPMENT CHECKLIST WANAY  SRT-73 2/4' x 2" FI. Green  RESPIRATORY CARE DEPT. EQUIPMENT CHECKLIST WANAY  SRT-73 2/4' x 2" FI. Green  RESPIRATORY CARE DEPT. EQUIPMENT CHECKLIST WANAY  SRT-74 3'4' x 2" FI. Green  RESPIRATORY CARE DEPT. EQUIPMENT CHECKLIST WANAY  SRT-75 1'x 2" FI. Green  RESPIRATORY CARE DEPT. RESPIRATORY CAR			
RESPIRATORY CARE DEPT. Check by date  SRT-76 2' x 3" FI. Red  Check by date  SRT-76 2' x 3" FI. Red  Check by date  Date  Date  Date  RESPIRATORY CARE DEPT. CLEAN AND ASSEMBLED RESPIRATORY CARE DEPT. CLEAN AND ASSEMBLED RESPIRATORY CARE DEPT. CLEAN COndition By:  Date  RESPIRATORY CARE DEPT. CLEAN AND ASSEMBLED RESPIRATORY CARE DEPT. CLEAN COndition By:  Date  RESPIRATORY SERVICES EQUIPMENT REPAIR  EQ. NO  DATE  RESPIRATORY SERVICES EQUIPMENT REPAIR  EQ. NO  DATE  REPAIR NEEDED  REPAIR NEEDED	SRT-44 3/4" x 4" FI. Red Perf Down Center For Easy Fold Over  Respiratory Use Only SRT-71 7/8" x 3"  RESPIRATORY CARE DEPT. EQUIPMENT CHANGED DATE INITIAL	VENTILATOR SETUP CHECKLIST CALIBRATION DONE ALARMS FUNCTIONING PRESSURE CHECK VOLUME CHECK FULTERS IN PLACE THERMOMETER VENTILATION MONITOR PAPERWORK SELF TEST PASSED VENT. I.D. # THERAPIST INITIALS DATE MISSING	VENTILATOR CHECKLIST VENT. I.D.#  FUNCTION TECH. A. CLEANING  B. REASSEMBLY  C. TEST RUN D. COMMENTS:  DATE:
Respiratory Care Dept. Emergency Equipment Break seal when needed Notify respiratory care when used  Check by	EQUIPMENT CHECKED  THIS ITEM IS NOT DISPOSABLE	REMOVED FROM AERATOR  AT : PM ON •••  BY	ASSEMBLED AND CHECKED By Date
Check by	Emergency Equipment  Break seal when needed	RETURN TO RESPIRATORY CARE	CAUTION EMPTY CYLINDER
DO NOT USE  Date: By: Problem:		CLEAN AND ASSEMBLED BY DATE EXP. DATE	This Unit Assembled In CLEAN Condition  By: Date:
Peel and Stick to Device.	DO NOT USE  Date: By:	EQUIPMEI EQ. NO. REPAIR NEEDED	NT REPAIR  DATE
SRT-42 3" x 3" 1,000 per roll SRT-43 3" x 5" 1,000 per roll			ECH

## **Shamrock Products for Color Coding**



#### SHAMROCK LABELING TAPE

- · 2 Lengths: 500", 2160"
- 5 Widths: ½" (ST-12), ¾" (ST-34), 1" (ST-10), 1½" (ST-11), 2" (ST-20)
- · 31 Distinct Colors

Ideal for color coding, Shamrock Labeling Tape accepts handwritten notations, sticks tightly, leaves no residue when removed and can be transferred from surface to surface. Call for information on tape imprinted to your specifications.



#### SHAMROCK DOT LABELS

#### · 6 Sizes:


<sup>1</sup>/<sub>4</sub>" (SDL-25), <sup>7</sup>/<sub>16</sub>" (SDL-43), <sup>1</sup>/<sub>2</sub>" (SDL-50), <sup>3</sup>/<sub>4</sub>" (SDL-75), 1" (SDL-100), 1<sup>1</sup>/<sub>4</sub>" (SDL-125)

#### • 31 Distinct Colors

Versatile Shamrock Dot Labels offer multiple opportunities for color coding and can be imprinted to your specifications. They are supplied on sheets or in roll form. Permanent adhesive is standard; removable adhesive is available upon request. Dots are supplied 1,000 per roll or 1,000 per package of individual sheets.



#### 31 DISTINCT COLORS



#### TAPE DISPENSERS



Easy to fill multiple dispensers offer convenient access from a central location.

#### HAND DISPENSERS



Durable plastic, can be reused many times.



## Terms and Conditions of Sale

All prices subject to change without notice.

A \$25.00 minimum order is required.

Prices are F.O.B. Bellwood, Illinois, unless otherwise specified. Foreign import duties and exchange rates, if any, are additional.

Terms: Net 30 days.

#### **RETURN POLICY**

No returns will be accepted without prior authorization. Shamrock's numbered return authorization form must accompany all merchandise returned.

**Defective Merchandise:** Should any Shamrock product prove to be defective, a claim for return must be placed within 60 days of shipment. Products shown to be defective and returned within this period will be replaced.

**Stock Items:** No return of stock items will be accepted after six months. A 15% restocking charge is imposed on return of all stock items.

Custom Items: Custom orders may not be returned.

#### **QUANTITIES**

Over runs or under runs, not to exceed 10% of quantities ordered, will constitute acceptable delivery.

#### **PLATE CHARGES**

Due to natural deterioration of printing plates, and in order to provide only topquality products, Shamrock must remake its plates every three years. If an order is not placed within that time, a new plate charge must be made upon receipt of the next order.







813



## **SHAMROCK LABELS**

34 Davis Drive, Bellwood, Illinois 60104

National Toll Free: 800-323-0249

California Toll Free: 877-461-6908

Fax Toll Free: 800-248-1907

Email: sales@shamrocklabels.com

Shop Online: shamrocklabels.com